



Certificate of Analysis

[Close](#)

COA Key >

2505140

Reported Date >

January 9, 2026



Authentic Results
results shall be open and transparent.



Accurate Reports
Accurate data, verified multiple times



Quality You Can Trust
Rigorous testing. Reliable results.

Sample

Glow Blend 10/10/50mg

Batch

25051

Sample description >

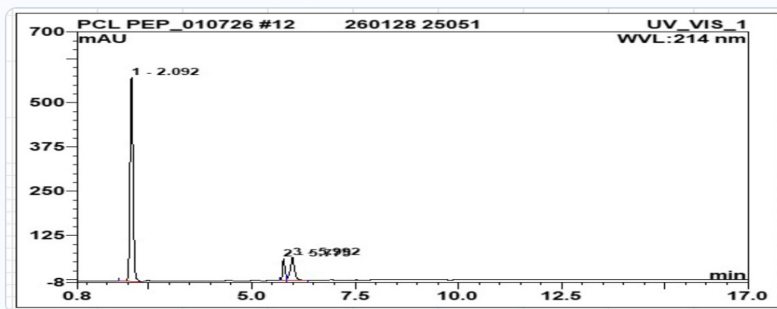
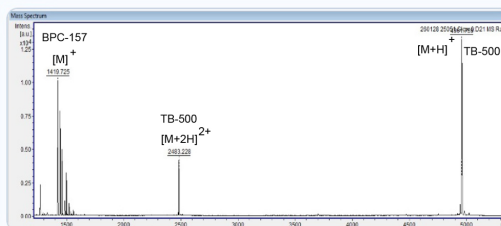
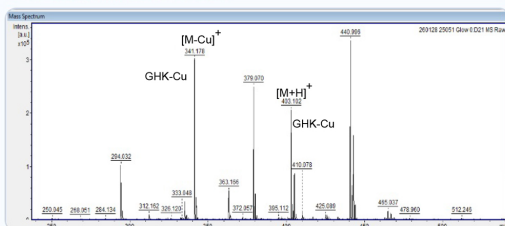
See picture or pictures attached.

**Tests requested >**

Assessment of a peptide vial or vials.

TEST RESULTS

Specification	Result	Method	Status
Identity: BPC-157, TB-500 & GHK-Cu	BPC-157, TB-500 & GHK-Cu	MALDI-MS	✓ Conforms
Content	10.12, 9.95 & 50.23 mg	HPLC Quantitation	✓ Conforms
Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms

ANALYTICAL DATA**HPLC Chromatogram (Retention Time: 5.7, 5.9 & 2.092 min)****Mass Spectrum (MALDI-MS)****Research and Formulation Chemist**

This purity analysis was conducted using UPLC/MS under standard laboratory conditions, following validated analytical protocols to ensure accurate and reliable results. This analysis is intended for informational and research applications.